

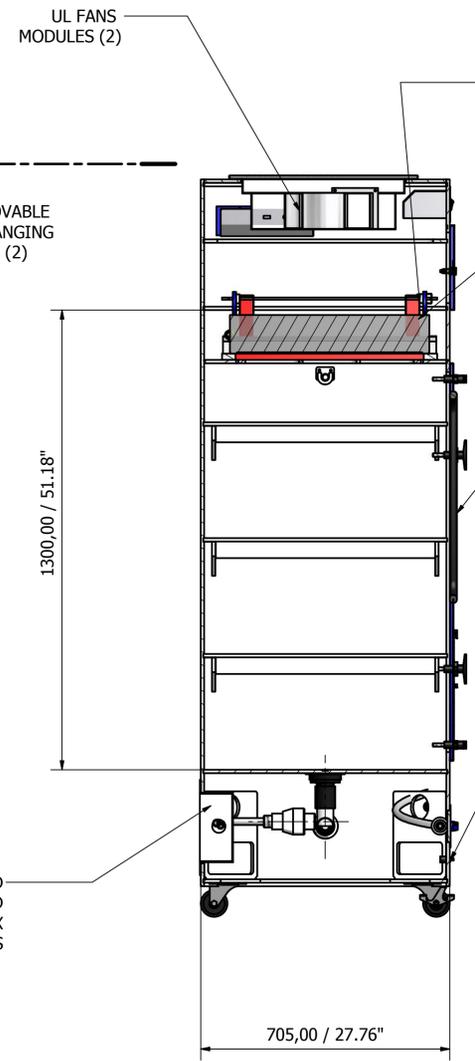
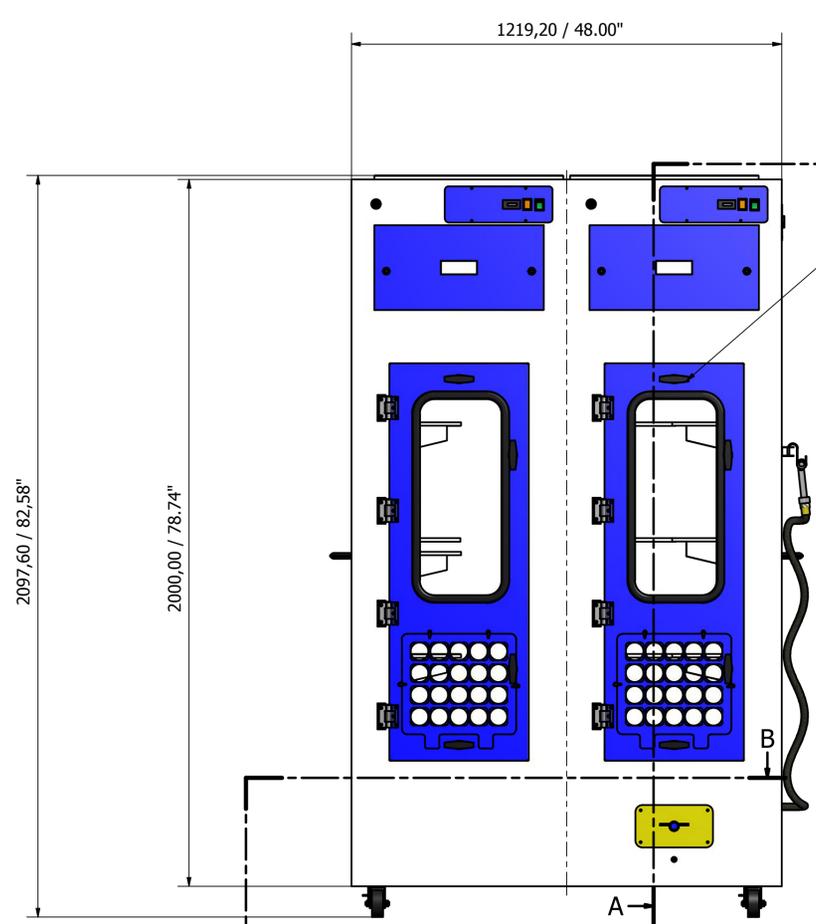


REVISION HISTORY				
ZONE	REV	DESCRIPTION	DATE	APPROVED
FAN LEVEL	1	UL FAN MODULE	7/06/2010	P CH
MAIN FILTER	2	METAL CLAMPS	8/12/2011	P CH
RIGHT SIDE	3	METAL SHOEBOX	3/18/2012	P CH
TOP COVER	4	UL FAN METAL MODULE	11/8/2017	P CH

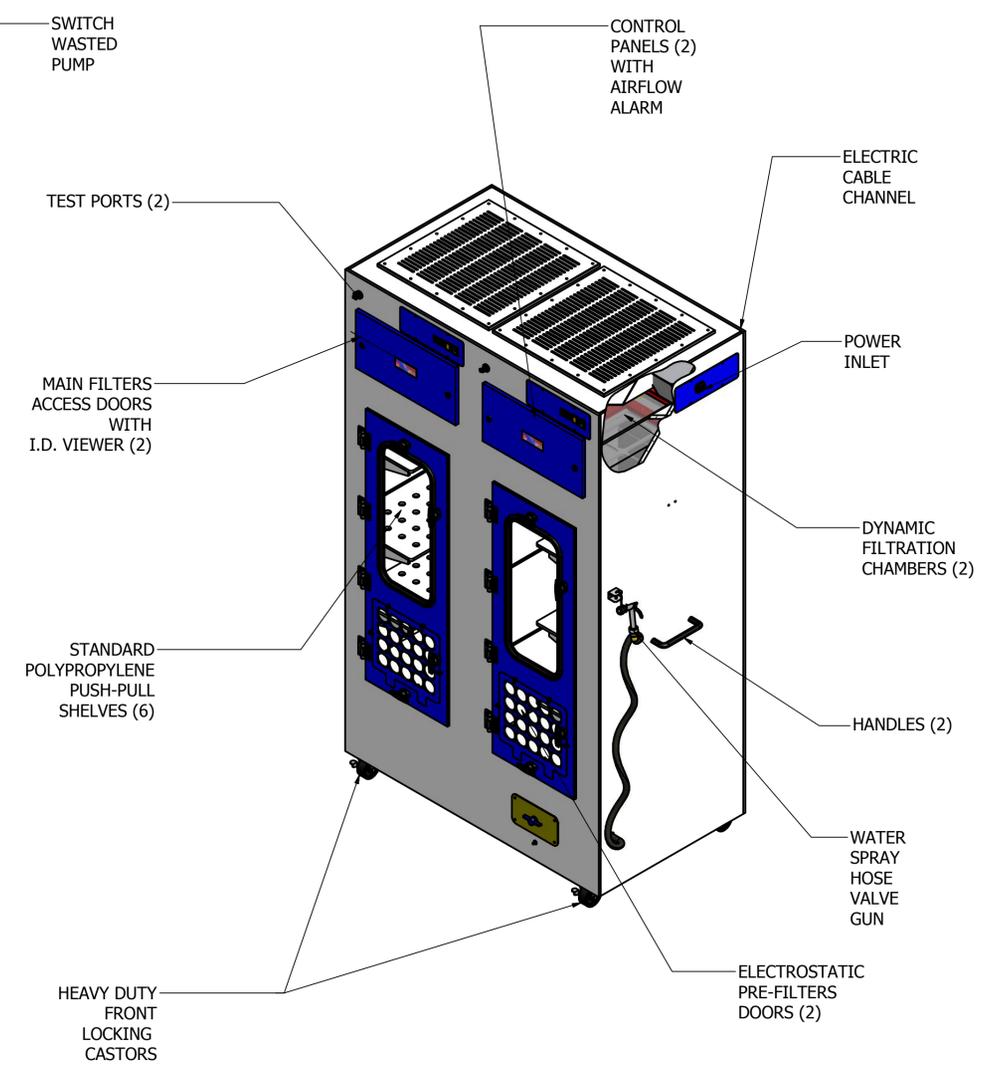

- NOTES:**
- 1.0 CUSTOMER:
 - 2.0 SUBMIT DRAWINGS FOR APPROVAL.
 - 3.0 INCLUDED:
 - 3.1 STANDARD ITEMS APPLIED.
 - 3.2 PLUMBING PACKAGE.
 - 3.3 SPRAY VALVE AND 1/2" X 6' HOSES FOR DRAINAGE AND COLD WATER WITH BRONZE FEMALE CONNECTORS.
 - 4.0 CABINET BUILT WITH 3/8" WHITE POLYPROPYLENE, SEAMLESS, NON-POROUS WATERTIGHT INSIDE, THERMALLY FUSE.
 - 5.0 STANDARD MOLDED PLUG NEMA 4-14P
 - 6.0 ELECTRICAL REQUIREMENTS 110V 6A 60 HZ

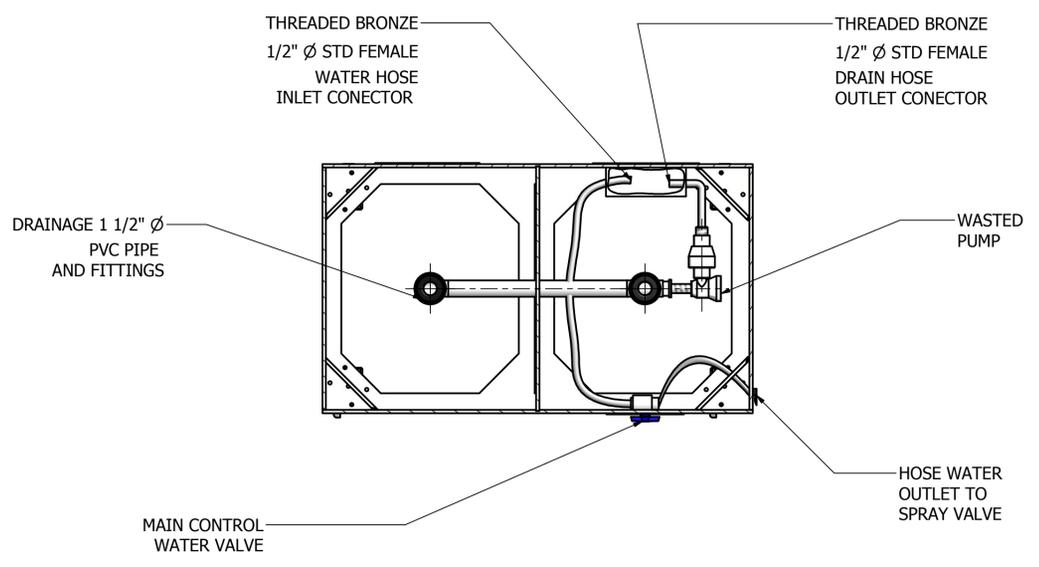

A-A (1 : 10)

B-B (1 : 10)

Designed by CFG	Checked by	Approved by	Date 11/9/2012	Date
AIR SCIENCE USA			DCD48XT-2000UL	
DCD48.UL-GAssem			Edition 4	Sheet 1 / 1